
# smartGAS.



### SILAREX

NDIR Multi-Gas Sensor CO<sub>2</sub> 20 Vol.-% // CO 10000 ppm smartGAS item number: SX-200004-00000

- 2 active measurement channels
- Ready to use calibrated
- On board cross compensation
- On board pressure compensation
- Modbus ASCII/RTU, autobaud, autoframe
- Status indicated by LED

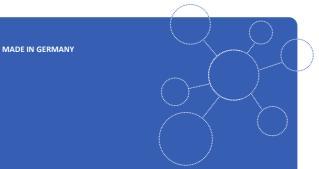

Application Examples Emission monitoring CEMS Biogas Process measurement Fruit ripening High voltage Available as 2-Channel 3-Channel

#### Accessories

Insulation housing Gas cooler Particle filter Gas pump Mounting equipment Available design in support Mechanical Installation Data communication Gas pre-treatment

smartGAS Mikrosensorik GmbH | Huenderstr. 1 | 74080 Heilbronn | Germany T +49 7131 797553-0 | F +49 7131 797553-10 | <u>sales@smartgas.eu</u> | <u>www.smartgas.eu</u>

# smartGAS.

#### SILAREX I CO2 // CO I SX-200004-00000

General featurs		Channel 1:	Channel 2:
Measurement principle:	Non Dispersive Infra-Red (NDIR), dual wavelength		
Target gas:		CO <sub>2</sub>	CO
Measurement range:	0 Full Scale (FS)	FS = 20 Vol%	FS = 10000 ppm
Gas supply:	by flow (nearly atmospheric pressure)		
Flow rate:	0.1 1.0 l / min		
Mounting dimensions:	336 mm x 30 mm x 50 mm (L x W x H)		
Warm-up time:	< 2 minutes (start up time) < 30 minutes (full specification)		
Measuring response*			
Response time (t <sub>90</sub> ) @ 0.7 l / min:	< 4 s (fast), < 8 s (medium), < 60 s (slow)		
Digital resolution:		0.01 Vol%	1 ppm
Detection limit (3 $\sigma$ ) max.:	in fast / medium / slow mode:	0.03 Vol% / 0.02 Vol% / 0.01 Vol%	6 ppm / 4 ppm / 2 ppm
Repeatability:		≤±0.06 Vol%	≤±6ppm
Linearity error (straight line deviation):		≤±0.1 Vol%	≤ ± 10 ppm
Long term stability (zero):	after 1000 h operating time	≤ ± 0.01 Vol%	≤±5 ppm
Long term stability (span):	after 1000 h operating time	≤ ± 0.02 Vol%	≤±8 ppm
Influence of T, P, flow rate, other	*		
Temp. dependence (zero):	with thermal isolation, heater on	≤ ± 0.005 Vol% per °C	≤±0.1 ppm per °C
Temp. dependence (span):	with thermal isolation, heater on	≤±0.01 Vol% per °C	≤±0.2 ppm per °C
Pressure dependence:	pressure compensated, residual error in % of actual reading / hPa	≤±0.02	≤±0.02
Flow rate dependence per 0.1 l / min:		≤±0.02 Vol%	≤±2 ppm
Cross sensitivity (zero) other gases:	@ 20 Vol% $CO_2$ (compensated for 42 °C): @ 10000 ppm CO (compensated for 42 °C):	- ≤±0.30 Vol%	< ± 120 ppm -
Electrical inputs and outputs			
Supply voltage:	24 V DC <u>+</u> 10 %		
Average power consumption	< 6 W (while heater on) // < 1 W (at stabilized temperature)		
Inrush current:	< 400 mA		
Digital output signal	Modbus ASCII / RTU via RS485, autobaud, autoframe		
Calibration	Zero and Span via Modbus ASCII / RTU		
Climatic conditions			
Sensor heating temperature	42 °C		
Operating ambient temperature:	appr. + 10 + 40 °C (thermal isolation required)		
Storage temperature:	-20 °C + 60 °C		
Air pressure:	800 1150 hPa		
Ambient humidity:	0 95 % rel. H. (not condensing)		

### \* Typical values related to 1013 hPa, Ta = 22 °C, flow = 0.7 l / min for dry (not condensing) and clean sample gas. Stated values exclude calibration gas tolerance.

All rights reserved. Any logos and/or product names are trademarks of smartGAS. The reproduction, transfer, distribution or storage of information contained in this brochure in any form without the prior written consent of smartGAS is strictly prohibited. All specifications – technical included – are subject to change without notice. Depending on the application, the target gas and the measurement range the technical data may differ. No liability is accepted for any consequential losses, injury or damage resulting from the use of this document or from any omissions or errors herein. The data is given for guidance only. It does not constitute a specification or an offer for sale.

For more information, please visit www.smartgas.eu or contact us at sales@smartgas.eu

Please consult smartGAS sales for parts specified with other temperature and measurement ranges. At first initiation and depending on application and ambient conditions recalibration is recommended. Recurring cycles of recalibration are recommended.